

A new method for
Tear Volume Measurement

SMTube®

Strip Meniscometry Tube


5 seconds

Dry eye screening

Five seconds quantification for
the lower tear meniscus volume



ECHO ELECTRICITY CO.,LTD.

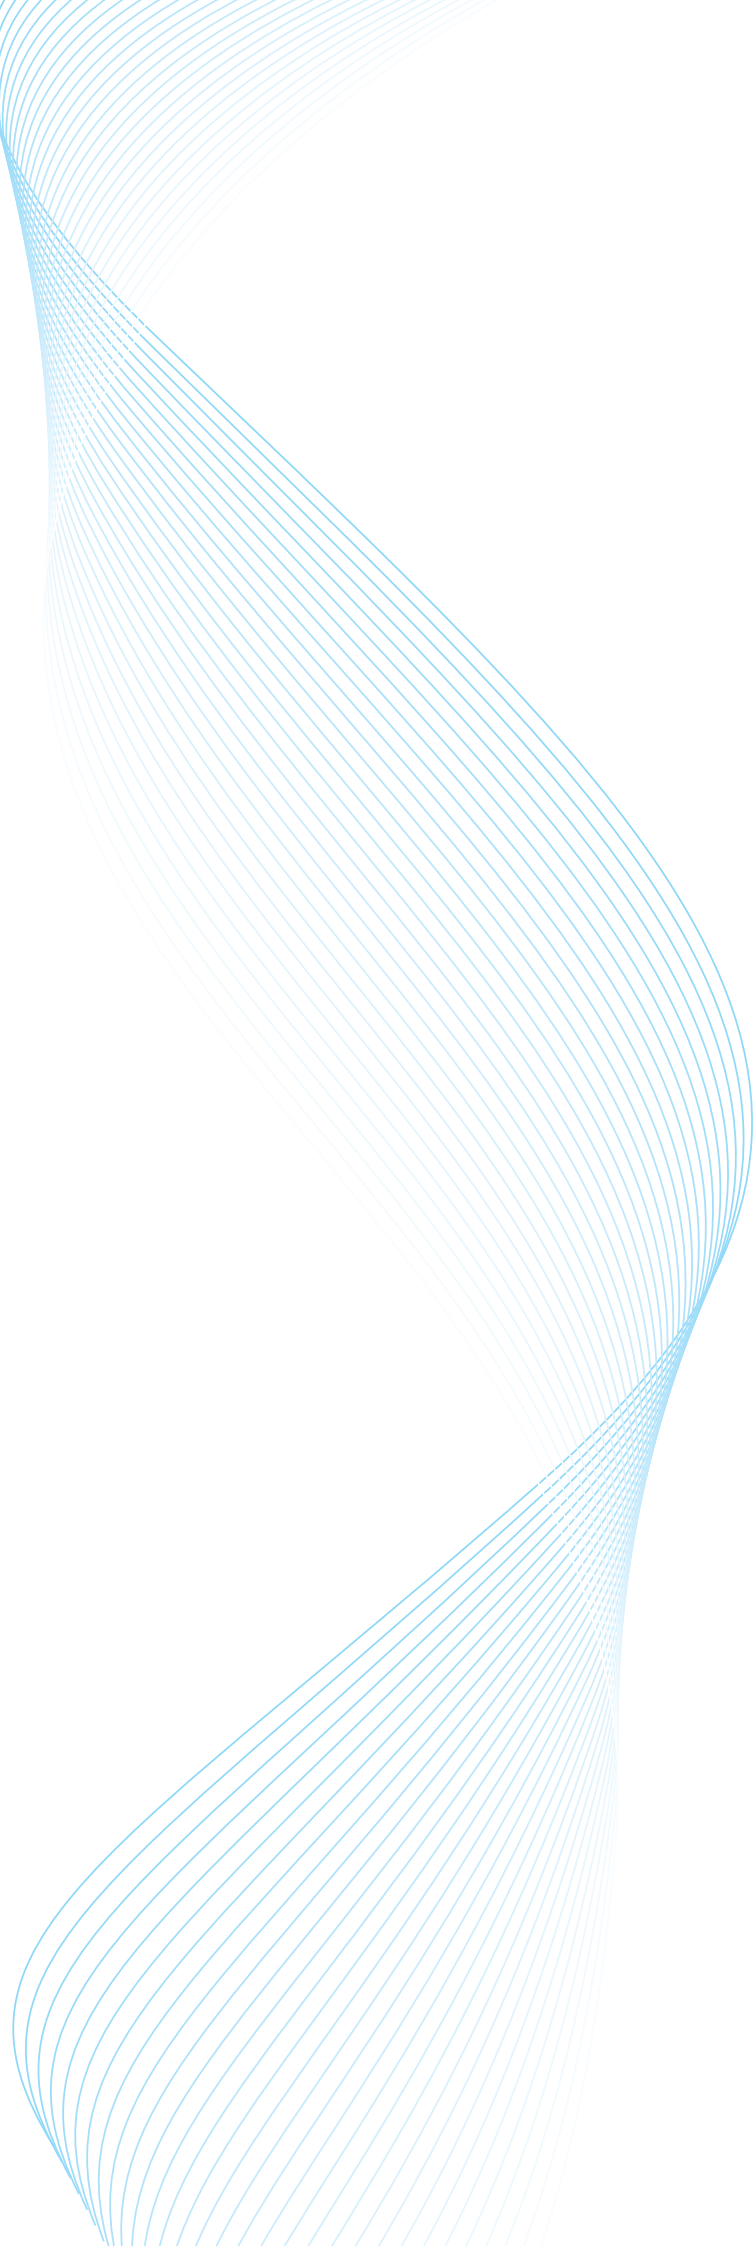

The tear film stability is closely related to the tear volume. Thus, the tear volume is an important parameter to conduct tear-film-oriented-therapy properly, where the treatment of dry eye disease or the postoperative care for refractive and cataract surgeries are typical examples of such.

In this brochure, we would like to introduce our new diagnostic medical device, "Strip Meniscometry Tube (SMTube)", developed for a simple, accurate, swift and minimally-invasive assessment of tear volume. "Strip Meniscometry" is a term of a methodology for the tear volume evaluation, of which the original paper was published in 2006 (Dogru 2006). Then in 2011, it has been reported that the strip meniscometry testing was useful in the diagnosis of dry eye disease, showing a statistically significant correlation with other ocular surface examinations such as the Schirmer test, tear film breakup time measurement, and vital staining scores (Ibrahim 2011).

"SMTube" is a product to perform the strip meniscometry testing, developed with an appropriate standardization and mass-production techniques, with intent to help medical staff carry out the testing with ease and accuracy.

All you do is to immerse the tip of the SMTube strip into the tear meniscus of the lower eyelid for 5 seconds. And column will be stained with blue dye as the SMTube absorbs tears. The length of stained column quantifies the tear meniscus volume.

Since SMTube is used right on ocular surfaces, the safety is highly considered; The material and structure were carefully chosen and designed so that no damage ought to occur on the ocular surface in case the tip of the strip touches cornea or conjunctiva.

A number of reports have been published in terms of the use of SMTube in their clinical studies (please see the reference papers on page 9 of this brochure).


Here are some of the examples :

1. Quantitative measurement of tear meniscus volume during visual field testings using SMTube (Sagara et al.)
2. An efficacy of SMTube testing in a mass screening of dry eye disease during regular medical checkup (Ishikawa 2018)
3. A clinical efficacy of SMTube in the diagnosis of dry eye disease when combined with OCT examinations (Shinzawa 2018)


Configuration / Structure

SMTube is thin strip with a central ditch filled with absorber. Scale is printed on the both sides of absorber to measure the tear meniscus volume. Each SMTube is packaged individually in sterile pouch.

Shape

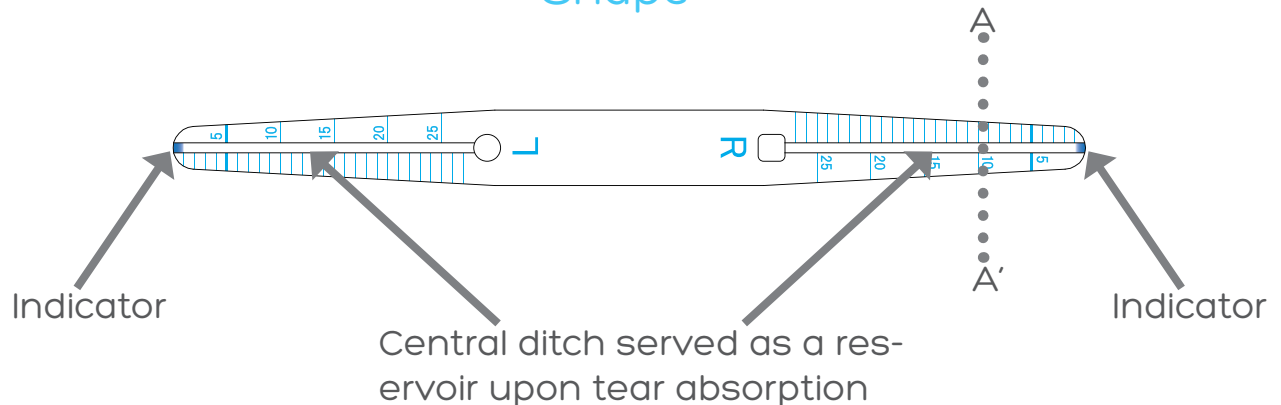

A - A' cross section

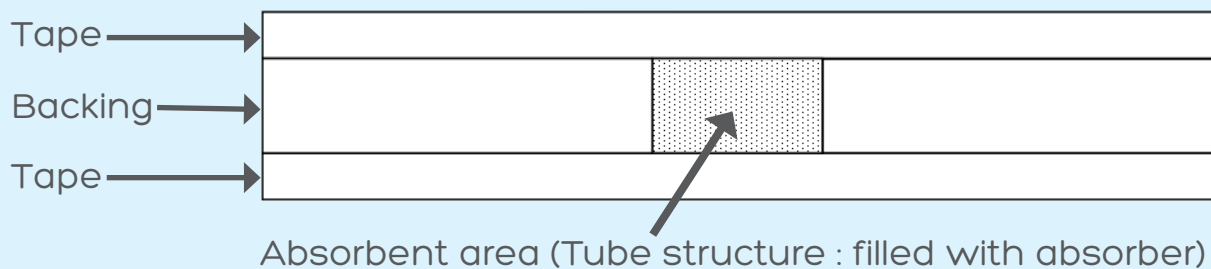

Size : Length : 85mm
Width : 7mm
Height : 0.3mm

Material : Indicator : Blue dye 1
Tape : Polyurethane, Polyester
Backing : Polyurethane
Absorber : Rayon, Pulp

When SMTube is applied to the tear meniscus in a lateral lower lid of an eye, it absorbs tears via the capillary action of absorber taking effect in the center of the strip. The indicator, placed at the end of the strip, is dissolved in the absorbed tear fluid. At the end of 5 seconds, the length of the stained tear column is marked and read to quantify the tear meniscus volume.



Single use only

Instruction for use


Without slitlamp (when used by paramedical staff)




Hold the center of SMTube strip.
Do not touch a tip of strip to avoid
potential infections.




Take the standing position with
the patient as shown in the left
photo. Fix the hand on the cheek
of patient, so that the tip of SM-
Tube is stabilized.

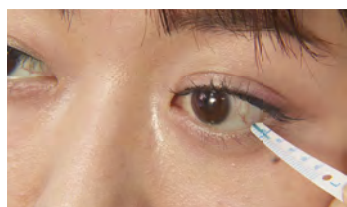

Immerse the tip of the L side into
the tear meniscus of the left lower
eyelid for 5 seconds to absorb
tears.
Take extra care not to touch the
conjunctiva nor the cornea with
the tip of the strip.

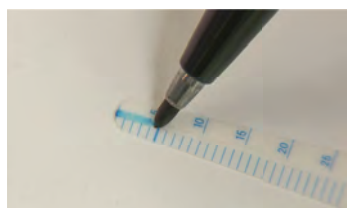

Read the score (length of the col-
umn stained by blue colour). Mark
with an oil pen if necessary.

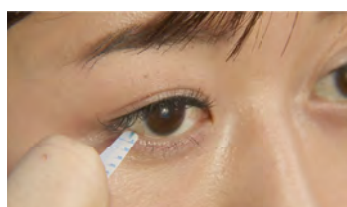

Switch to the R side of the strip,
and perform the testing on the
right eye in the same manner as
done on the left eye.


With slitlamp (when used by doctors)



Make sure to use the illumination
with an essentially-minimum in-
tensity to avoid the reflex secretion
caused by the photostimulation.
Use a diffuser if available.



Perform the testing on the left eye
using the L side of the strip.

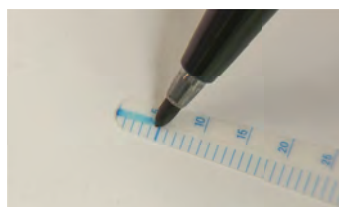

Read the score (length of the col-
umn stained by blue colour). Mark
with an oil pen if necessary.



Switch to the R side of the strip,
and perform the testing on the
right eye. We recommend to fix
the hand as shown in the left
photo.

Hold a strip as follows

Make sure to hold the center part of SMTube during the examination. SMTube absorbs tears by capillary action, and holding the column parts or blocking the hole near the central of the strip (the end of the column) may disturb the capillary action.




Angle of Instertion

The angle of instertion is highly important in order to evaluate tear meniscus volume correctly.

The good example shown in the picutre below is showing that stirip is inserted into tear meniscus, with correct anlge.


The bad example shown the picurre below is showing that the strip is applied with a too downward angle, which may cause the failure on absobtion, or inaccurate evaluation score.

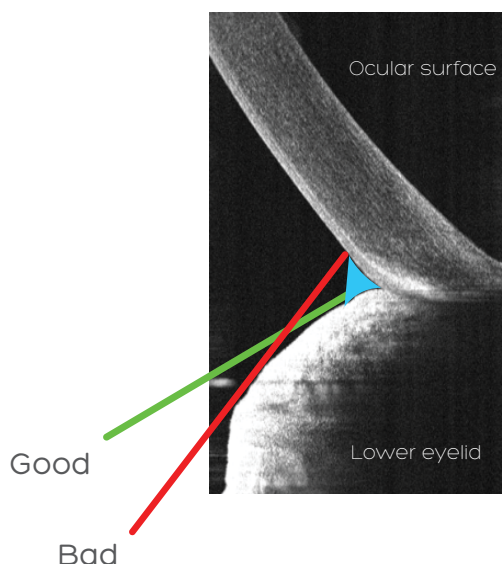

Contraindications




When taking out the strip, do not touch the tip of SMTube strip where the blue dye is impregnated.

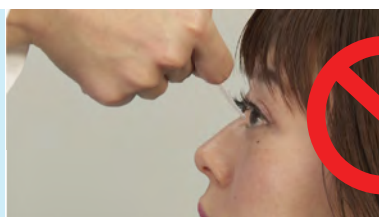

Please note that when applying the strip, keep the appropriate angle near the horizontal. In an example on the left, the strip is applied with a too upward angle.




Do not block the hole near the center of the strip (the end of the column) during the examination. Blocking the hole will disturb the capillary action.

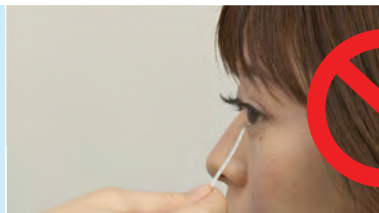

Please note that when applying the strip, keep the appropriate angle near the horizontal. In an example on the left, the strip is applied with a too downward angle.



Never touch the cornea with the strip.


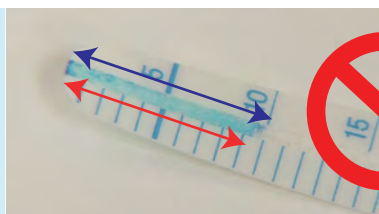


When reading the score, adopt the highest value (indicated by a blue arrow) instead of the shortest value (indicated by a red arrow) or so.



Do not deform or apply a pressure upon eyelid during the examination.

Comparison with the Schirmer's test

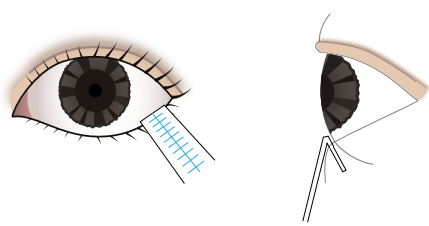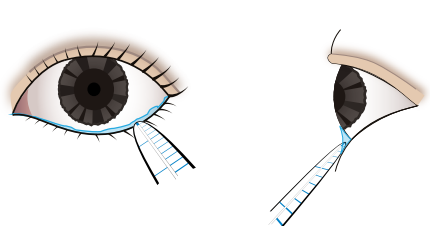	 <p>The Schirmer's test</p>	 <p>SMTube®</p>
Usage	Inserting the Schirmer strip inside the lower eyelid (conjunctival sac)	Immersing the tip of SMTube strip into the tear meniscus
Required time	5 minutes	5 seconds x 2 (for both eyes)
Invasiveness	invasive	Minimally-invasive

SMTube has a high correlation with OCT

A clinical trial has proved that the SMTube testing has a high correlation with the Schirmer test, tear meniscus height (TMH) and area (TMA) measurements using an optical coherence tomography (OCT), and tear film breakup time (BUT) measurement (Shinzawa 2015).

In this study, subjects were comprised of definite dry eye group and healthy control group. The detail is summarized in Fig.1 below.

Fig.2 below is a table demonstrating the correlation among the examinations. The diagonal cells are for the examination entries. The lower triangular cells exhibit scatter plots between the scores, and the upper triangular cells represent the correlation coefficients between the scores calculated by the Spearman's rank test.


Figure 1 : Summary of Subjects

Diagnosis	Subjects (eyes)	Gender *		Age Range (yrs)	Mean Age* (yrs)
		Men (eyes)	Women (eyes)		
DE	23 (45)	5 (10)	18 (35)	8-86	56.4 ± 17.0
Normal Controls	29 (51)	7 (11)	22 (40)	7-82	53.6 ± 18.4

Subjects with dry eye symptoms, presence of a vital staining score of >3points, and decreased tear break-up time or tear quantity were diagnosed as having definite dry eye disease according to the 2006 Japanese Dry Eye Research Society Diagnostic Criteria.


*No statistically significant differences were found in terms of male-female ratio ($P = 1.0$ with Fisher's exact test, $P = 0.90$ with the chi-square test with Yates' correction) and the age distribution ($P = 0.61$ with Mann-Whitney U test).

Figure 2 : Correlation among SMTube and other ocular surface examinations

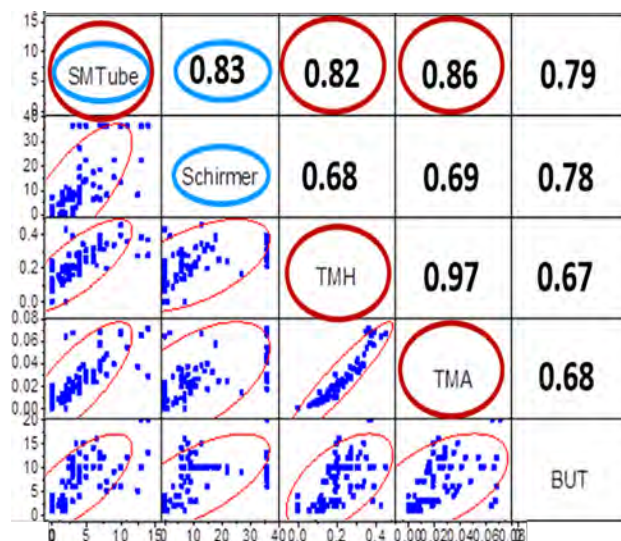

Tear meniscus assessment using OCT has recently attracted a lot of attention due to its non-invasiveness, swiftness and accuracy upon the evaluation of tear meniscus parameters including height, area, volume as well as curvature, where the tear meniscus volume is regarded to be the most essential. SMTube allows you to perform the tear meniscus volume evaluation without restrictions in terms of the cost, time, and place owing to its inexpensiveness and portability. An evidence of the high correlation between SMTube with OCT invokes that SMTube can be utilized for the tear volume measurement instead of using an expensive OCT instrument.

An estimate for cut-off length

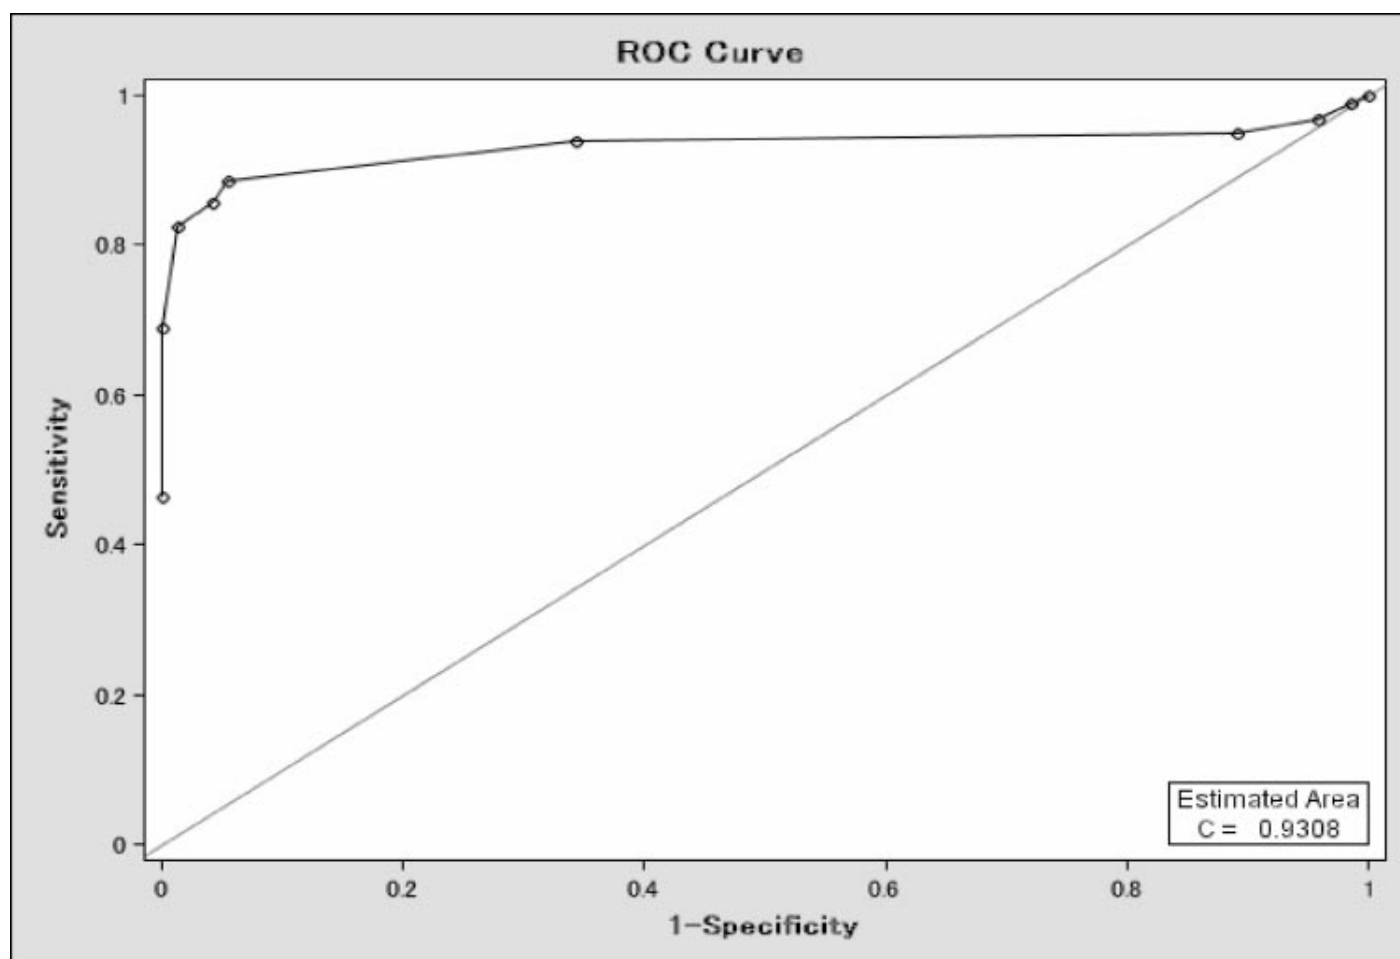

Cut-off value (mm):	<1	<2	<3	<4	<5	<6	<7	<8	<10	>=10
Sensitivity:	0.46	0.69	0.82	0.86	0.89	0.94	0.95	0.97	0.99	1.00
Specificity:	1.00	1.00	0.99	0.96	0.95	0.66	0.11	0.04	0.01	0.00

The ROC graph showing the sensitivity and specificity of strip meniscometry test. (Dogru 2006)

Combinations of diagnostic tests may help to diagnose DE syndrome more accurately

The study demonstrated the efficacy, safety, and efficiency of SM and DEQS for the screening of DE syndrome during general medical checkup in a large population. The combination of SM and DEQS for diagnosis of DE yielded high sensitivity and specificity, indicating its feasibility for the screening of DE syndrome. (Ishikawa 2018)

Sensitivity and specificity of dry eye-related quality-of-life score, strip meniscometry score.

Examination (number of cases)	Sensitivity, %	Specificity, %
DEQS (n= 54, DE group=28 normal group=26)	79	91
SM (n=70, DE group=24 normal group=46)	71	85
Single positive (DEQS or SM) (n=103, DE group=33, normal group=70)	97	77
Double positive (DEQS and SM) (n=28, DE group=20, normal group=8)	59	97

DE=dry eye, DEQS=dry eye-related quality-of-life score, SM=strip meniscometry.

Comparison of mean values of DED parameters (Shinzawa 2018)

Ocular Surface Test	DED, n=43 Eyes	Controls, n=49 Eyes
OSDI	36.0±27.2 (0–93.2)	11.4±13.0 (0–68.8) ^a
DEQS	34.9±22.0 (5–83.3)	9.8±13.6 (0–50.0) ^a
SMTube, mm	1.4±2.3 (0–13)	5.5±2.8 (2–14) ^a
OCT-TMH, mm	0.138±0.102 (0–0.426)	0.271±0.108 (0.132–0.685) ^a
OCT-TMA, mm ²	0.013±0.015 (0–0.067)	0.033±0.025 (0.007–0.152) ^a
BUT, sec	2.4±1.2 (1–6)	10.0±2.5 (6–16) ^a
Schirmer, mm	1.7±3.0 (0–11)	17.1±11.4 (6–36) ^a
FS	5.2±2.0 (1–9)	0.0±0.0 (0–0) ^a
LS	6.1±2.1 (3–9)	0.0±0.0 (0–0) ^a

Values are given as mean ± SD (range).

Statistically significant differences were found by Mann–Whitney *U* test ($P < 0.001$).

DED, dry eye disease; OSDI, Ocular Surface Disease Index; DEQS, Dry Eye–related Quality-of-life Score; SMTube, Strip Meniscometry Tube; OCT, optical coherence tomography; TMH, tear meniscus height; TMA, tear meniscus area; BUT, break-up time; FS, fluorescein; LS, lissamine green.

Application of SMTube

The advantage of SMTube is its swiftness and handiness in measuring tear volume without requiring special equipments. For this reason, SMTube is suitable for the first screening test of dry eye diagnosis, to differentiate true ADDE (Aqueous Deficient Dry Eye) from EDE (Evaporative Dry Eye). The applicable circumstance of exploiting the advantage of SMTube is not only for dry eye diagnosis. It can be applied not only as a “short-time” and “minimally invasive” tear volume measurement, but it can also be applied as a convenient tool for various purposes required in various clinical sites and researches.

- 1. Screening of a number of subjects such as group health checkup. (Ishikawa 2018)**
- 2. Examining the amount of tears before and after a certain treatment and medication. (Ibrahim 2012, Kojima 2014, Okura 2015)**
- 3. Monitoring the time-series variation of the tear volume, which is repeated in short period of time. (Kojima 2011, Hirayama 2013, Sano 2015, Ayaki 2019)**
- 4. It is suitable for tear volume evaluation in pediatrics, owing to its minimal invasiveness.**
- 5. Initial screening to rule out normal eyes from KCS in dogs. (Miyasaka 2019)**

Product Information

Pouch : Each SMTube is individually sterilized

Package : 50 strips/box



- PCT patented
- European Medical Device Directive 93/42/EEC, CE marked as Class I
- FDA device registered as Class I
- MHLW Japan registered as Class I medical device

References

Original Papers

- Dogru M, Ishida K, Matsumoto Y, Goto E, Ishioka M, Kojima T, Goto T, Saeki M, Tsubota K. Strip meniscometry: a new and simple method of tear meniscus evaluation. *Invest Ophthalmol Vis Sci.* 2006; 47: 1895-1901.
- Ibrahim OM, Dogru M, Ward SK, Matsumoto Y, Wakamatsu TH, Ishida K, Tsuyama A, Kojima T, Shimazaki J, Tsubota K. The efficacy, sensitivity, and specificity of strip meniscometry in conjunction with tear function tests in the assessment of tear meniscus. *Invest Ophthalmol Vis Sci.* 2011; 52: 2194-2198.
- Lee KW, Kim JY, Chin HS, Seo KY, Kim TI, Jung JW. Assessment of the Tear Meniscus by Strip Meniscometry and Keratograph in Patients With Dry Eye Disease According to the Presence of Meibomian Gland Dysfunction. *Cornea.* 2017; 36: 189-195.
- Ishikawa S, Takeuchi M, Kato N. The combination of strip meniscometry and dry eye-related quality-of-life score is useful for dry eye screening during health checkup: Cross-sectional study. *Medicine (Baltimore).* 2018; 97: e12969.
- Shinzawa M, Dogru M, Miyasaka K, Shimazaki J, Sekiryu T. Application of CASIA SS-1000 Optical Coherence Tomography Tear Meniscus Imaging in Testing the Efficacy of New Strip Meniscometry in Dry Eye Diagnosis. *Eye Contact Lens.* 2018; 44 Suppl 1: S44-S49.
- Ayaki M, Tachi N, Hashimoto Y, Kawashima M, Tsubota K, Negishi K. Diurnal variation of human tear meniscus volume measured with tear strip meniscometry self-examination. *PLoS One.* 2019; 14: e0215922.
- Shinzawa M, Dogru M, Miyasaka K, Kojima T, Tsubota K. The Application of Strip Meniscometry to the Evaluation of Tear Volume in Mice. *Invest Ophthalmol Vis Sci.* 2019; 60: 2088-2091.
- Alshammeri S, Madden L, Hagan S, Pearce EI. Strip meniscometry tube: a rapid method for assessing aqueous deficient dry eye. *Clin Exp Optom.* 2019.
- Sagara H, Sekiryu T, Imaizumi K, Shintake H, Sugiyama U, Maehara H. Impact of tear metrics on the reliability of perimetry in patients with dry eye. *PLoS One.* 2019; 14: e0222467.
- Singh A, Vanathi M, Kishore A, Gupta N, Tandon R. Evaluation of strip meniscometry, tear meniscus height and depth in the diagnosis of dry eye disease in asian Indian eyes. *Ocul Surf.* 2019; 17: 747-752.
- Ishikawa S, Shoji T, Yamada N, Shinoda K. Efficacy of Strip Meniscometry for Detecting Lacrimal Obstructive Diseases Among Patients With Epiphora. *Transl Vis Sci Technol.* 2019; 8: 8.

References

Original papers in Veterinary

Rajaei SM, Ansari Mood M, Asadi F, Rajabian MR, Aghajanzpour L. Strip meniscometry in dogs, cats, and rabbits. *Vet Ophthalmol.* 2018; 21: 210-213.

Miyasaka K, Kazama Y, Iwashita H, Wakaiki S, Saito A. A novel strip meniscometry method for measuring aqueous tear volume in dogs: Clinical correlations with the Schirmer tear and phenol red thread tests. *Vet Ophthalmol.* 2019.

Peer-reviewed papers using SM in study

Ibrahim OM, Dogru M, Takano Y, Satake Y, Wakamatsu TH, Fukagawa K, Tsubota K, Fujishima H. Application of visante optical coherence tomography tear meniscus height measurement in the diagnosis of dry eye disease. *Ophthalmology.* 2010; 117: 1923-1929.

Dogru M, Ward SK, Wakamatsu T, Ibrahim O, Schnider C, Kojima T, Matsumoto Y, Ogawa J, Shimazaki J, Tsubota K. The effects of 2 week senofilcon-A silicone hydrogel contact lens daily wear on tear functions and ocular surface health status. *Cont Lens Anterior Eye.* 2011; 34: 77-82.

Kojima T, Matsumoto Y, Ibrahim OM, Wakamatsu TH, Uchino M, Fukagawa K, Ogawa J, Dogru M, Negishi K, Tsubota K. Effect of controlled adverse chamber environment exposure on tear functions in silicon hydrogel and hydrogel soft contact lens wearers. *Invest Ophthalmol Vis Sci.* 2011; 52: 8811-8817.

Ibrahim OM, Dogru M, Kojima T, Matsumoto Y, Wakamatsu TH, Tsubota K, Fujishima H. OCT assessment of tear meniscus after punctal occlusion in dry eye disease. *Optom Vis Sci.* 2012; 89: E770-E776.

Hirayama M, Murat D, Liu Y, Kojima T, Kawakita T, Tsubota K. Efficacy of a novel moist cool air device in office workers with dry eye disease. *Acta Ophthalmol.* 2013; 91: 756-762.

Ibrahim OM, Dogru M, Kawashima S, Wakamatsu TH, Tsubota K, Fujishima H. Visante optical coherence tomography and tear function test evaluation of cholinergic treatment response in patients with sjogren syndrome. *Cornea.* 2013; 32: 653-657.

Kojima T, Matsumoto Y, Ibrahim OM, Wakamatsu TH, Dogru M, Tsubota K. Evaluation of a thermosensitive atelocollagen punctal plug treatment for dry eye disease. *Am J Ophthalmol.* 2014; 157: 311-317.

Sano K, Kawashima M, Ikeura K, Arita R, Tsubota K. Abdominal breathing increases tear secretion in healthy women. *Ocul Surf.* 2015; 13: 82-87.

Okura M, Kawashima M, Katagiri M, Shirasawa T, Tsubota K. New Eye Cleansing Product Improves Makeup-Related Ocular Problems. *J Ophthalmol.* 2015; 2015: 831628.

Raposo AC, Portela RD, Masmali A, Cardoso-Brito V, Bernardo M, Oliveira DC, Oria AP. Evaluation of lacrimal production, osmolarity, crystallization, proteomic profile, and biochemistry of capuchin monkeys' tear film. *J Med Primatol.* 2018.

Others (proceeding / article / book)

Ibrahim OM. Strip Meniscometry. In: Yokoi N (ed), *Ophthalmic Care Qualification for Specialists: A Road to the Dry Eye Specialist*; Nakayama Shoten; 2013:171-174. (in Japanese)

Ishikawa S, Kato N, Okamoto Y, Takeuchi D. 健康診断におけるStrip Meniscometryを用いた涙液量検査の有用性: Utility of tear volume measurement using strip meniscometry at a mass medical checkup. *Annual Meeting of Japanese Society of Lacrimal Passage and Tear Dynamics.* Tokyo: Session Number RR-7-1; 2014. (in Japanese)

Shinzawa M, Dogru M, Miyasaka K, Shimazaki J, Sekiryu T. 前眼部OCTとstrip meniscometryのドライアイ診断への応用: Application of Anterior-Segment OCT and strip meniscometry in the diagnosis of dry eye. *J Jpn Ophthalmol Soc.* 2015;119(Suppl.):212. (in Japanese)


Shinzawa M, Dogru M, Miyasaka K, Shimazaki J, Sekiryu T. Application of OCT Tear Meniscus Imaging and New Strip Meniscometry in the Diagnosis of Dry Eye Disease. *Invest Ophthalmol Vis Sci.* 2015; 56(special issue): 293.

Sagara H. Quantitative Measurement of Tear Meniscus Volume during Visual Field Testing with Strip Meniscometry. 6th World Glaucoma Congress. Hong Kong: Session Number P-T-057; 2015.

Ishikawa S, Kato N, Takeuchi M. The Efficacy of Strip Meniscometry and DEQS for Dry Eye Screening during Medical Health checkups. Poster Session in ARVO (Poster Board Number: A0061); 2016.

Miyasaka K, Kazama Y, Iwashita H, Saito A. CLINICAL EFFICACY OF A NEW QUICK TEAR VOLUME MEASUREMENT IN DOGS: STRIP MENISCOMETRY. General Scientific Session in ACVO (Baltimore); 2017.

Thank you.

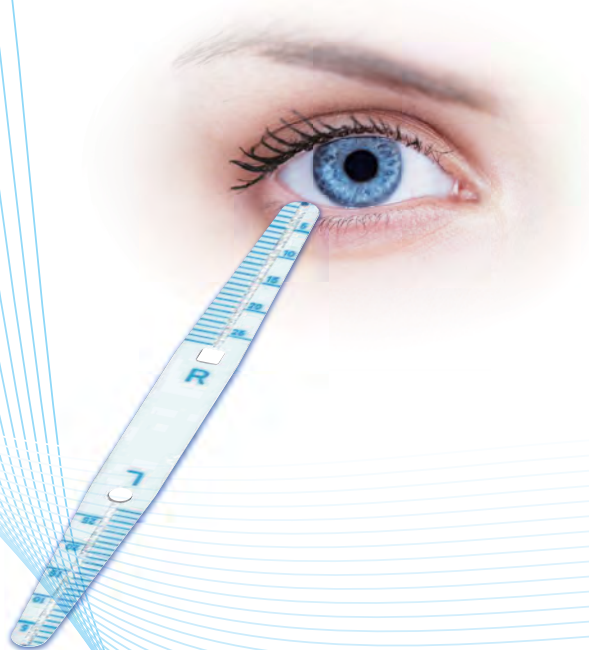

Our SMTube technical documents are available@
<http://www.echo-mf.jp/en/smtube/product/>



ECHO ELECTRICITY CO.,LTD.

PRODUCT INQUIRIES : TOKYO OFFICE

6-24-14 Umeda Adachi-ku Tokyo 123-0851 Japan

PHONE : +81 3 3880 0455 FAX : +81 3 3848 1825

URL : <http://www.echo-mf.jp/en.html>

EMAIL : contact-english@echo-mf.jp

MANUFACTURER : SHIRAKAWA FACTORY

1-2 Shinnatsunashi Shirakawa-shi Fukushima-ken 961-0024 Japan

- ISO 13485:2016 / JIS Q 13485:2018 certified
- Medical devices manufacturer licensed by MHLW Japan
- MHLW third-class medical devices marketing authorization holder
- FDA registration



JQA-MD0220
Manufacture of LACRIMAL Tube
(Head office (Shirakawa Factory))

09APR2025